Injection Date : 9/23/97 8:15:10 PM Seq. Line : 35
Sample Name : 000945152880 Vial : 35
Acq. Operator : martinj Inj : 1
Inj Volume : 1 µl

Acq. Method : C:\HPCHEM\1\METHODS\H2O.M
Last changed : 9/23/97 11:43:59 AM by martinj
Analysis Method : C:\HPCHEM\1\METHODS\NIC.M
Last changed : 10/3/97 10:41:00 AM
(modified after loading)
Water Analysis - Routine Nicotine and Water Analysis

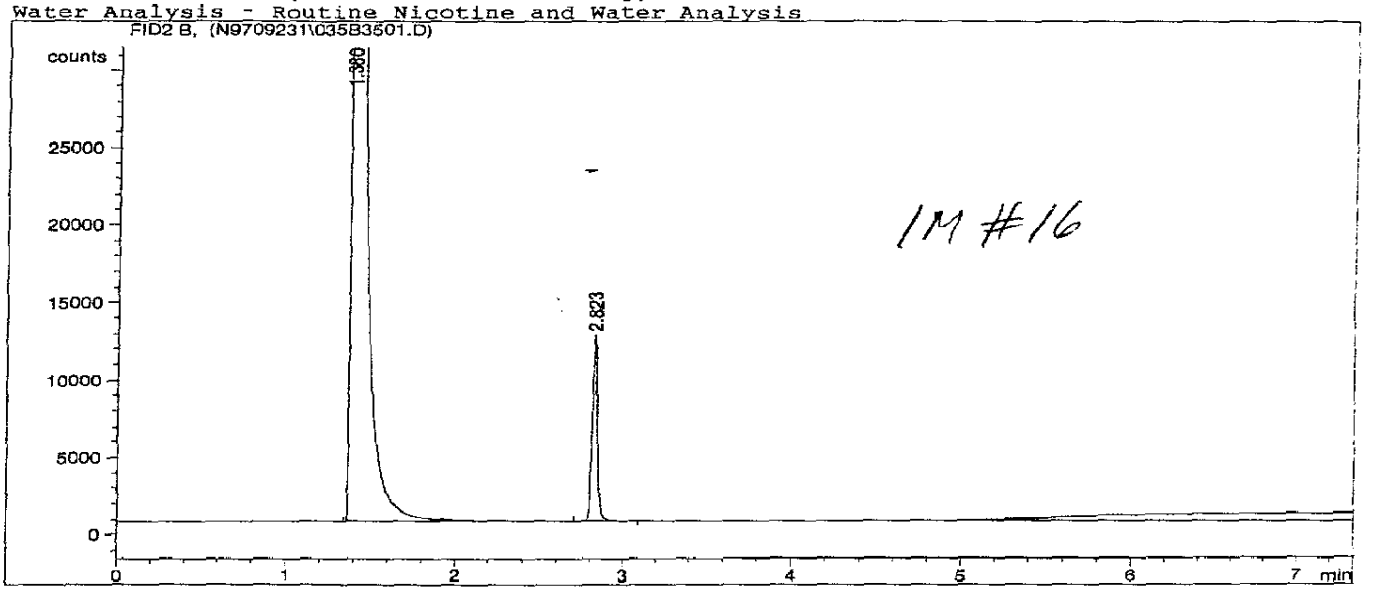


IM #16

Internal Standard Report (Sample Amount is 0!)

Sorted By : Signal
Calib. Data Modified : 10/3/97 10:35:20 AM
Multiplier : 1.0000
Dilution : 1.0000
Uncalibrated Peaks : not reported

Sample ISTD Information:

| ISTD # | ISTD Amount [mg/cigt] | Name |
|---|---|---|
| 1 | 1.00000 | Carvone |

Signal 1: FID2 B,
Results obtained with enhanced integrator!

| RetTime [min] | Type | Area counts*s | Amt/Area ratio | Amount [mg/cigt] | Grp | Name |
|---|---|---|---|---|---|---|
| 2.823 | VV T+I | 2.74855e4 | 1.00000 | 1.00000 | | Carvone |
| 3.654 | | - | - | - | | Nic |

Totals without ISTD(s) : 0.00000

2 Warnings or Errors :

Warning : Time reference compound(s) not found
Warning : Sample amount is zero. Absolute amounts calculated



PM3000376374

Source: https://www.industrydocuments.ucsf.edu/docs/mlwl0001